SHENYUN

INSTRUCTIONS FOR USE

Medical-Grade Silicone Tubing

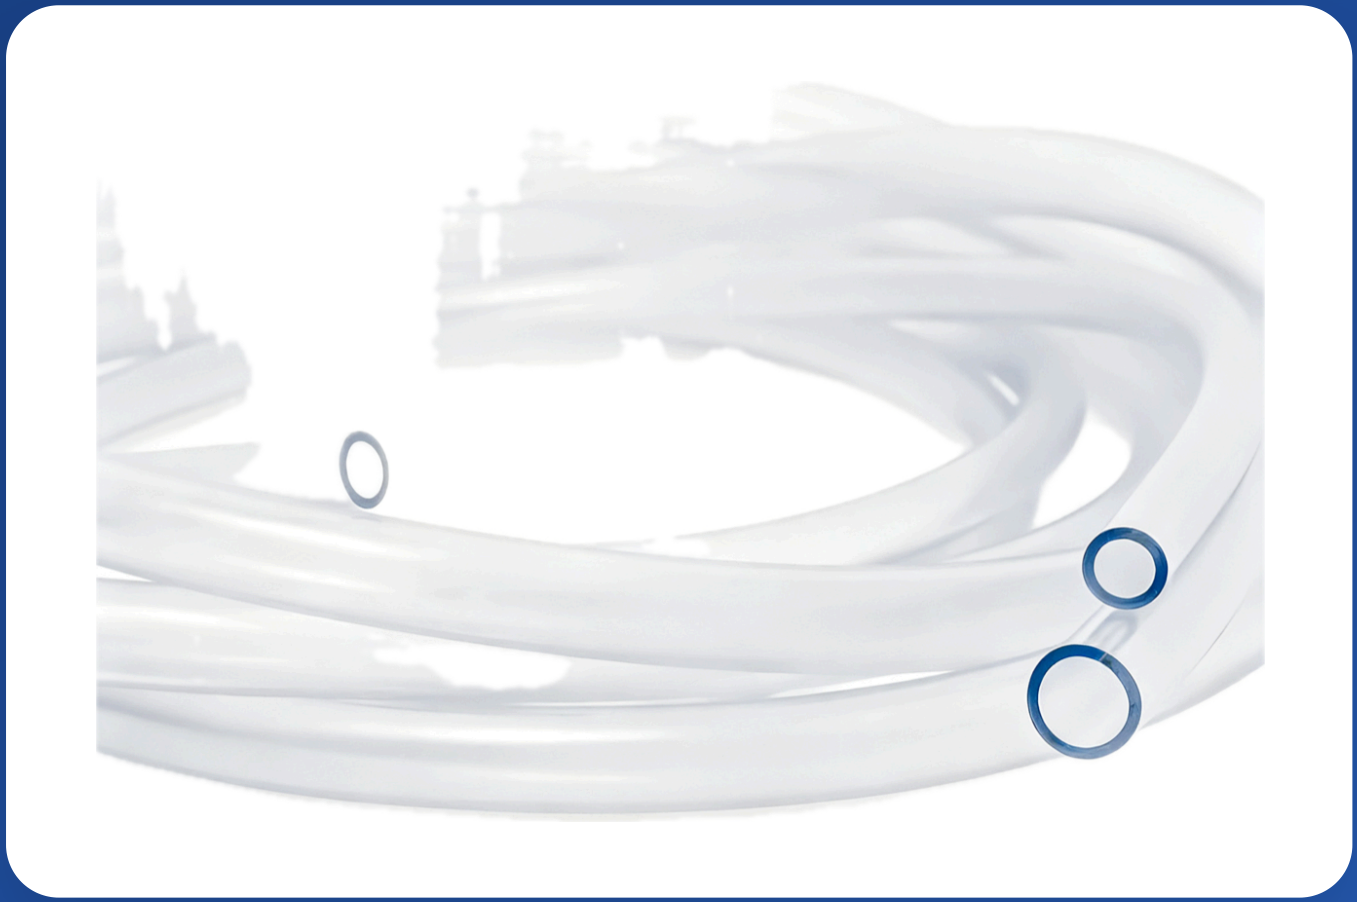

Suzhou Shenyun Medical Equipment Co., Ltd.
Building 11, No. 666 Yinzang Road, Linhu Town, Wuzhong District, Suzhou, Jiangsu, China
info@symedical.com.cn · www.sybariatric.com

SHENYUN
Suzhou Shenyun Medical Equipment Co., Ltd.

info@symedical.com.cn
Tel / WhatsApp +86 151 5045 7575
www.sybariatric.com

INSTRUCTIONS FOR USE

Medical-Grade Silicone Tubing

1. PRODUCT INFORMATION

Platinum-cured medical-grade silicone tubing, 31 standard sizes MST-001 – MST-031, ID 0.5–12.0 mm, OD 1.3–18.5 mm; custom sizes on request. See the technical data sheet for the full size list.



2. INTENDED PURPOSE

Non-invasive medical applications in hospitals and similar settings, such as connecting medical equipment, and laboratory use. Not intended for delivering fluids into, or draining fluids from, the human body.

3. INTENDED USERS AND ENVIRONMENT

- Intended users: healthcare and laboratory professionals, and manufacturers using the tubing as a component.
- Intended environment: hospitals, laboratories and production facilities.

4. CONTRAINDICATIONS

Do not use for delivering fluids into, or draining fluids from, the human body.

5. WARNINGS AND PRECAUTIONS

- Check the tubing for damage, contamination or foreign matter before use; do not use if defective.
- Use clean tools to cut the tubing to length; avoid sharp edges that may damage the tube.
- Avoid strong oxidising agents and organic solvents, which may cause swelling or damage.
- Where sterilization or disinfection is required, the user is responsible for validating the process for the intended application.

6. INSTRUCTIONS FOR USE

1. Select the tubing size (ID and OD) for the connectors to be used.
2. Cut to the required length with clean tools.
3. Push the tubing fully onto the connectors and check that all connections are secure and free of kinks.

7. STORAGE

- Store in the original packaging in a clean, dry place away from direct sunlight, ignition sources and strong oxidising agents.
- Batch number: see the product label.

8. DISPOSAL

Dispose of according to local regulations; tubing contaminated by use should be treated as clinical waste.

9. SYMBOLS

	Refer to the instructions		No secondary use		Limit of stacking layers
	Keep dry		Batch code		Vertically upward
	Use-by date		Date of manufacture		Keep away from sunlight
	Unique device identifier		Manufacturer		Caution

Symbols according to ISO 15223-1:2021.

MANUFACTURER

Suzhou Shenyun Medical Equipment Co., Ltd.
Building 11, No. 666 Yinzang Road, Linhu Town, Wuzhong District,
Suzhou City, Jiangsu Province, P.R. China
SRN CN-MF-000026847
info@symedical.com.cn · www.sybariatric.com